
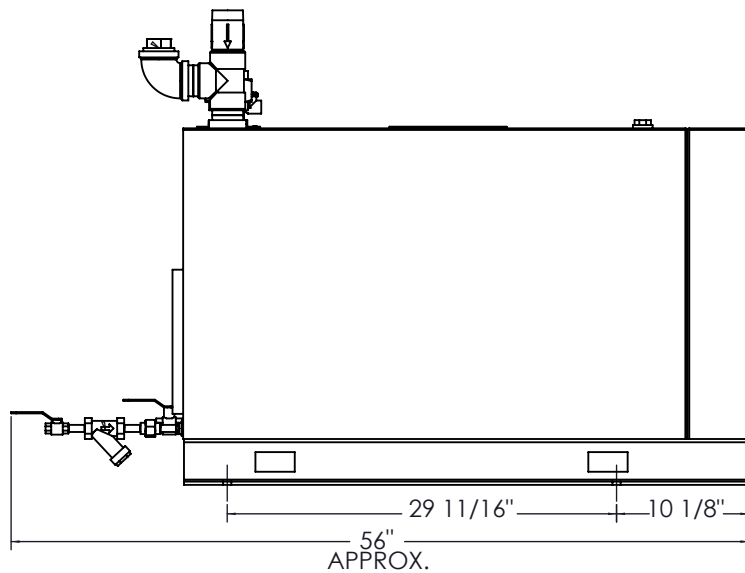



FOR INITIAL START-UP:
 ADD WATER TO THE SUMP
 THROUGH THIS CONNECTION
 UNTIL THE LEVEL REACHES THE
 LEVEL OF THE OVERFLOW ON
 THE BACK OF THE UNIT.

ADD 1.3 GALLONS OF WATER
 TO PRIME PUMP THE FIRST TIME
 UNIT IS BEING RUN.

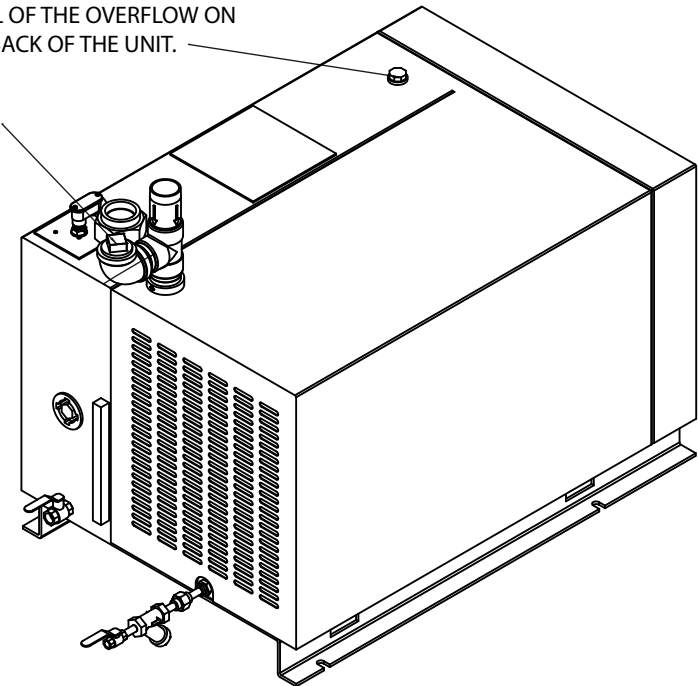

NOTE: PUMP MODULES ARE SHOWN WITH OPTIONAL EXTERNAL PIPING
 COMPONENTS FOR DIMENSIONAL PURPOSES.

01	N/A	INITIAL RELEASE	04/15/11	F.L.
REV	ECO NO.	DESCRIPTION OF CHANGE	DATE	BY
DO NOT SCALE DRAWING				
UNLESS OTHERWISE SPECIFIED: DIMENSIONS ARE IN INCHES AND TOLERANCES ARE		DRAWN BY	DATE	 <small>COPYRIGHT & COPYRIGHTED BY OHIO MEDICAL CORPORATION</small>
.XX ± 0.1 .XXX ± 0.01 XXX ± 0.005 XX ± .1		F. LOPEZ	04/15/11	
THIRD ANGLE PROJECTION		CHECKED BY	DATE	
MATERIAL:		APPROVED BY	DATE	
FINISH:		ITEM DESCRIPTION		
N/A		OASIS PUMP MODULE O200		
FILE NAME:		DWG SIZE	PART NUMBER	PART REV
100-0106.slddrw		D	301157	01
SCALE: 1:1			SHEET 1 OF 1	

CONFIDENTIAL: THIS DRAWING AND THE DESIGN REPRESENTED THEREIN ARE THE PROPERTY OF OHIO MEDICAL CORPORATION AND HAS BEEN ISSUED WITH THE UNDERSTANDING THAT NEITHER DRAWING NOR THE INFORMATION THEREIN IS TO BE USED OR DISCLOSED, EITHER IN WHOLE OR PART, EXCEPT AS SPECIFICALLY AUTHORIZED BY OHIO MEDICAL CORPORATION AND SHALL BE RETURNED UPON REQUEST.