

A1500-S3-V240 Reciprocating Medical Air System

System is NFPA compliant and has modular construction and interconnecting piping.

PUMP MODULE

The belt driven oil-less piston compressor delivers pressures up to 115 psi. Each module includes the compressor; motor; drive belts with belt guard; inlet filter; isolation valve; aftercooler; temperature switch for each cylinder, unloader solenoid, and relief valve.

AIR TREATMENT MODULE

The system's air treatment module features dual desiccant dryers configured for energy savings. They purge only when needed per the dew point setting. The dew point and CO transducers are integrated with the electrical panel. The module also contains prefilters, after filters, and activated carbon filters. Final line pressure regulators with gauges and relief valves are also part of the air treatment module.

AIR RECEIVER

The receiver is constructed to ASME standards and is galvanized for corrosion resistance. A source isolation valve and 3 valve bypasses are provided with the receiver module. A pressure gauge and relief valve are included, along with a sight window and electric auto drain. Mounting pads and flexible connectors are provided.

CONTROL PANEL

The UL listed electrical control panel features a high-definition color touch screen that can be set up externally without the use of toggle switches. The panel displays multiple conditions, including compressor running status, elapsed hours, pressure level, and audio/visual alarms.

Standard features include lag alarm, automatic compressor alternation, adjustable minimum run timer, adjustable pressure settings, adjustable screen brightness, alarm history registry, and data logging. The panel has standard dry contacts and Modbus interface with building management systems. Ethernet and BACnet are available as options. The panel's maintenance menu includes service items and maintenance warnings, and it is programmed for both English and Spanish languages.

Configuration	Triplex Stack Mount
System Capacity*	120 SCFM @ 50 psi 60 Hz. 100 SCFM @ 50 psi 50 Hz.
Horsepower (Each Pump)	15 HP
Horsepower (Total System)	45 HP
Available Voltage	208/230/460 v. 3 phase 60 Hz. 380 v. 3 phase 50 Hz. Contact Factory for other voltages
Full Load Amps 3 ph.	208 volts: 147 230 volts: 133.6 380 volts: 76.7 460 volts: 67
Tank Size	240 gallon vertical
Key Options	Bacterial filters for dryer/filter skid. Can be configured for lab use without lag alarm. Expandable for additional compressors.

Click here for compressor specifications and industry-leading parts support.





*System capacity is stated with one pump in reserve per NFPA. Capacity based on operation at sea level. For higher altitude, contact factory for adjusted capacity.

SYSTEM MODEL NO.	PART NO.	HP EACH	SCFM/ACFM @ 50 PSIG EACH	SCFM/ACFM @ 100 PSIG EACH	DESIGN CAPACITY (TR 50PSIG EACH)	RECEIVER SIZE (GALLONS)	PUMP DISCHARGE NPT	ESTIMATED SYSTEM WEIGHT (LBS)
A1500B-V24-DD	ADM1500(C)-440-53-V240-DD	15	55	55	114	240	1"	3100

SPACE ALLOWANCE FOR MAINTENANCE = 3 FT. ON ALL SIDES, MORE SPACE IS REQUIRED FOR THE OPENING OF LARGER PANEL DOORS.


TABLE 1		
SYSTEM LISTED ARE 440V. IF ANOTHER VOLTAGE IS REQUIRED, USE THE FOLLOWING PART NUMBERS.		
VOLTAGE	SYSTEM P/N	PUMP MODULE P/N
208-40-3	ADM1500(C)-208-53-V240-DD	100-0224
230-40-3	ADM1500(C)-230-53-V240-DD	100-0224
380-50-3	ADM1500(C)-380-53-V240-DD	100-0224

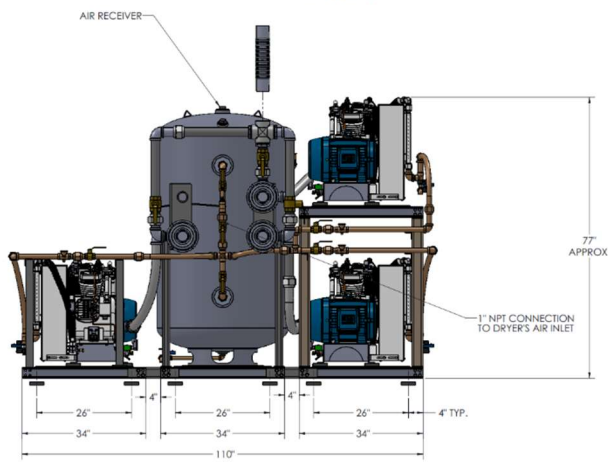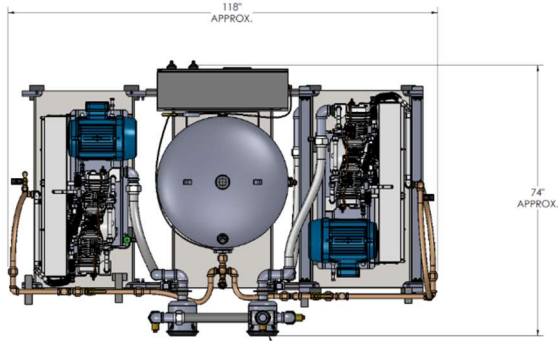

3" NPT AIR INLET CONNECTION

AIR COMPRESSOR MODULE

ELECTRICAL CONTROL PANEL

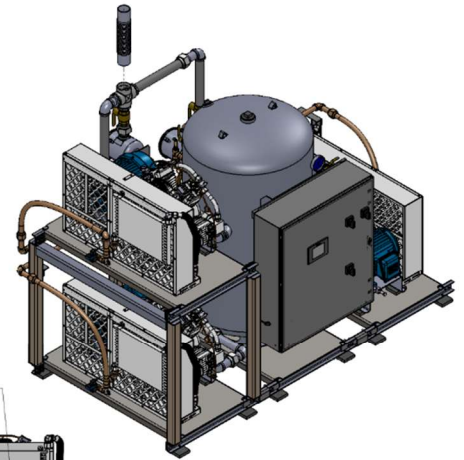

Q1	N/A	INITIAL RELEASE	01/01/19	FA
Q2	00140	DESCRIPTION OF DEVICE	001	BT
Q3	00140	REVISION	01/01/19	FA
Q4	00140	REVISION	01/01/19	FA
Q5	00140	REVISION	01/01/19	FA
Q6	00140	REVISION	01/01/19	FA
Q7	00140	REVISION	01/01/19	FA
Q8	00140	REVISION	01/01/19	FA
Q9	00140	REVISION	01/01/19	FA
Q10	00140	REVISION	01/01/19	FA
Q11	00140	REVISION	01/01/19	FA
Q12	00140	REVISION	01/01/19	FA
Q13	00140	REVISION	01/01/19	FA
Q14	00140	REVISION	01/01/19	FA
Q15	00140	REVISION	01/01/19	FA
Q16	00140	REVISION	01/01/19	FA
Q17	00140	REVISION	01/01/19	FA
Q18	00140	REVISION	01/01/19	FA
Q19	00140	REVISION	01/01/19	FA
Q20	00140	REVISION	01/01/19	FA
Q21	00140	REVISION	01/01/19	FA
Q22	00140	REVISION	01/01/19	FA
Q23	00140	REVISION	01/01/19	FA
Q24	00140	REVISION	01/01/19	FA
Q25	00140	REVISION	01/01/19	FA
Q26	00140	REVISION	01/01/19	FA
Q27	00140	REVISION	01/01/19	FA
Q28	00140	REVISION	01/01/19	FA
Q29	00140	REVISION	01/01/19	FA
Q30	00140	REVISION	01/01/19	FA
Q31	00140	REVISION	01/01/19	FA
Q32	00140	REVISION	01/01/19	FA
Q33	00140	REVISION	01/01/19	FA
Q34	00140	REVISION	01/01/19	FA
Q35	00140	REVISION	01/01/19	FA
Q36	00140	REVISION	01/01/19	FA
Q37	00140	REVISION	01/01/19	FA
Q38	00140	REVISION	01/01/19	FA
Q39	00140	REVISION	01/01/19	FA
Q40	00140	REVISION	01/01/19	FA
Q41	00140	REVISION	01/01/19	FA
Q42	00140	REVISION	01/01/19	FA
Q43	00140	REVISION	01/01/19	FA
Q44	00140	REVISION	01/01/19	FA
Q45	00140	REVISION	01/01/19	FA
Q46	00140	REVISION	01/01/19	FA
Q47	00140	REVISION	01/01/19	FA
Q48	00140	REVISION	01/01/19	FA
Q49	00140	REVISION	01/01/19	FA
Q50	00140	REVISION	01/01/19	FA
Q51	00140	REVISION	01/01/19	FA
Q52	00140	REVISION	01/01/19	FA
Q53	00140	REVISION	01/01/19	FA
Q54	00140	REVISION	01/01/19	FA
Q55	00140	REVISION	01/01/19	FA
Q56	00140	REVISION	01/01/19	FA
Q57	00140	REVISION	01/01/19	FA
Q58	00140	REVISION	01/01/19	FA
Q59	00140	REVISION	01/01/19	FA
Q60	00140	REVISION	01/01/19	FA
Q61	00140	REVISION	01/01/19	FA
Q62	00140	REVISION	01/01/19	FA
Q63	00140	REVISION	01/01/19	FA
Q64	00140	REVISION	01/01/19	FA
Q65	00140	REVISION	01/01/19	FA
Q66	00140	REVISION	01/01/19	FA
Q67	00140	REVISION	01/01/19	FA
Q68	00140	REVISION	01/01/19	FA
Q69	00140	REVISION	01/01/19	FA
Q70	00140	REVISION	01/01/19	FA
Q71	00140	REVISION	01/01/19	FA
Q72	00140	REVISION	01/01/19	FA
Q73	00140	REVISION	01/01/19	FA
Q74	00140	REVISION	01/01/19	FA
Q75	00140	REVISION	01/01/19	FA
Q76	00140	REVISION	01/01/19	FA
Q77	00140	REVISION	01/01/19	FA
Q78	00140	REVISION	01/01/19	FA
Q79	00140	REVISION	01/01/19	FA
Q80	00140	REVISION	01/01/19	FA
Q81	00140	REVISION	01/01/19	FA
Q82	00140	REVISION	01/01/19	FA
Q83	00140	REVISION	01/01/19	FA
Q84	00140	REVISION	01/01/19	FA
Q85	00140	REVISION	01/01/19	FA
Q86	00140	REVISION	01/01/19	FA
Q87	00140	REVISION	01/01/19	FA
Q88	00140	REVISION	01/01/19	FA
Q89	00140	REVISION	01/01/19	FA
Q90	00140	REVISION	01/01/19	FA
Q91	00140	REVISION	01/01/19	FA
Q92	00140	REVISION	01/01/19	FA
Q93	00140	REVISION	01/01/19	FA
Q94	00140	REVISION	01/01/19	FA
Q95	00140	REVISION	01/01/19	FA
Q96	00140	REVISION	01/01/19	FA
Q97	00140	REVISION	01/01/19	FA
Q98	00140	REVISION	01/01/19	FA
Q99	00140	REVISION	01/01/19	FA
Q100	00140	REVISION	01/01/19	FA

