

A2000-S3-V240 Reciprocating Medical Air System

System is NFPA compliant and has modular construction and interconnecting piping.

PUMP MODULE

The belt driven oil-less piston compressor delivers pressures up to 115 psi. Each module includes the compressor; motor; drive belts with belt guard; inlet filter; isolation valve; aftercooler; temperature switch for each cylinder, unloader solenoid, and relief valve.

AIR TREATMENT MODULE

The system's air treatment module features dual desiccant dryers configured for energy savings. They purge only when needed per the dew point setting. The dew point and CO transducers are integrated with the electrical panel. The module also contains prefilters, after filters, and activated carbon filters. Final line pressure regulators with gauges and relief valves are also part of the air treatment module.

AIR RECEIVER

The receiver is constructed to ASME standards and is galvanized for corrosion resistance. A source isolation valve and 3 valve bypasses are provided with the receiver module. A pressure gauge and relief valve are included, along with a sight window and electric auto drain. Mounting pads and flexible connectors are provided.

CONTROL PANEL

The UL listed electrical control panel features a high-definition color touch screen that can be set up externally without the use of toggle switches. The panel displays multiple conditions, including compressor running status, elapsed hours, pressure level, and audio/visual alarms.

Standard features include lag alarm, automatic compressor alternation, adjustable minimum run timer, adjustable pressure settings, adjustable screen brightness, alarm history registry, and data logging. The panel has standard dry contacts and Modbus interface with building management systems. Ethernet and BACnet are available as options. The panel's maintenance menu includes service items and maintenance warnings, and it is programmed for both English and Spanish languages.

Configuration	Triplex Stack Mount
System Capacity*	152 SCFM @ 50 psi 60 Hz. 126.6 SCFM @ 50 psi 50 Hz.
Horsepower (Each Pump)	20 HP
Horsepower (Total System)	60 HP
Available Voltage	208/230/460 v. 3 phase 60 Hz. 380 v. 3 phase 50 Hz. Contact Factory for other voltages
Full Load Amps 3 ph.	208 volts: 186.6 230 volts: 169.6 380 volts: 100.7 460 volts: 85
Tank Size	240 gallon vertical
Key Options	Bacterial filters for dryer/filter skid. Can be configured for lab use without lag alarm. Expandable for additional compressors.





Click here for compressor specifications and industry-leading parts support.



*System capacity is stated with one pump in reserve per NFPA. Capacity based on operation at sea level. For higher altitude, contact factory for adjusted capacity.

SYSTEM MODEL NO.	PART NO.	HP EACH	SCFM/ACFM @ 50 PSIG EACH	SCFM/ACFM @ 100 PSIG EACH	DESIGN CAPACITY (lb 50PSIG EACH)	RECEIVER SIZE (GALLONS)	PUMP DISCHARGE NPT	ESTIMATED SYSTEM WEIGHT (lb)
A2000B-53-DD	AOM2000-440-53-V240-DD	20	73.0	62.0	130.0	240	1"	6800

TABLE 1			
SYSTEM LISTED ARE 480V. IF ANOTHER VOLTAGE IS REQUIRED, USE THE FOLLOWING PART NUMBERS.			
VOLTAGE	SYSTEM P/N	PUMP MODULE P/N	TRIP MODULE P/N
208-40-3	ACM2000-208-53-V240-DD	100-0225	21453P
230-40-3	ACM2000-230-53-V240-DD	100-0225	21453P
380-50-3	ACM2000-380-53-V240-DD	100-0225	21454E

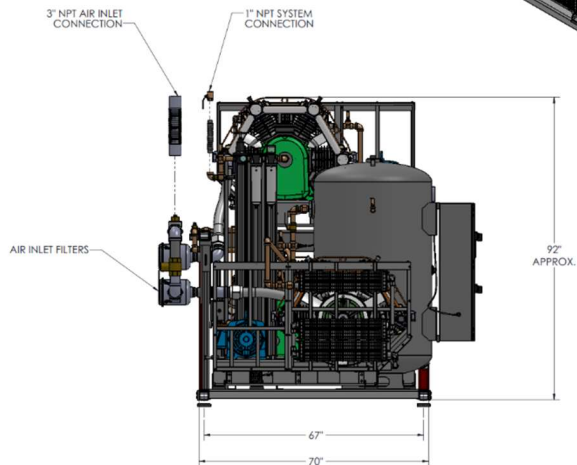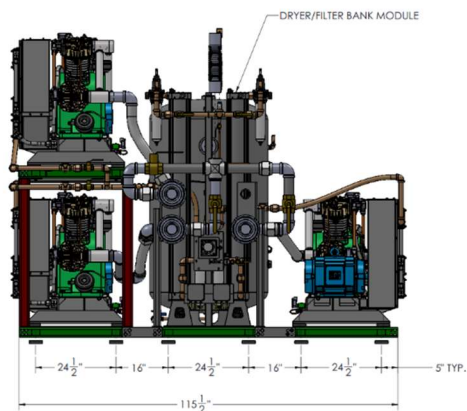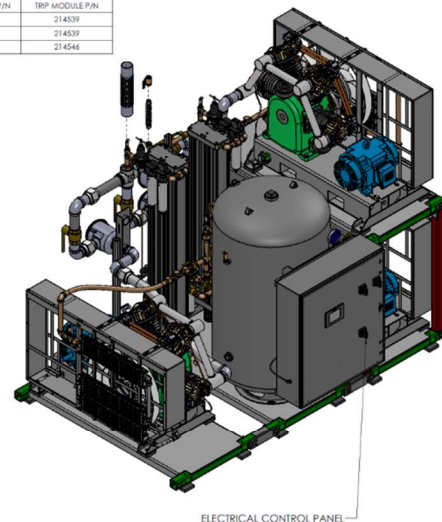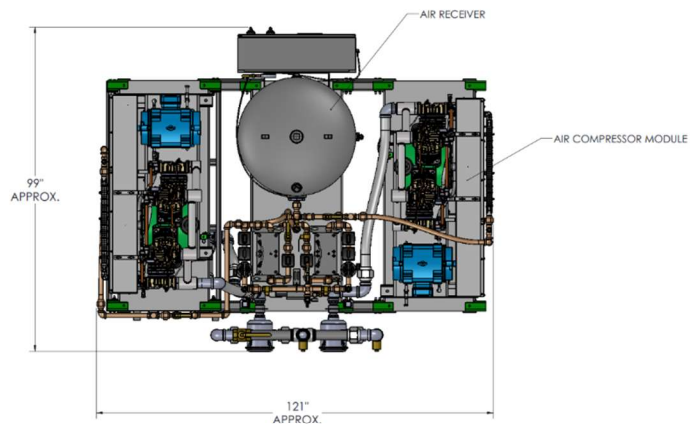

REV	DATE	DESCRIPTION OF CHANGE	BY	CHKD
1	05/09/13	INITIAL RELEASE	P. LOPEZ	
2	05/09/13	REVISION 1		
3	05/09/13	REVISION 2		
4	05/09/13	REVISION 3		
5	05/09/13	REVISION 4		
6	05/09/13	REVISION 5		
7	05/09/13	REVISION 6		
8	05/09/13	REVISION 7		
9	05/09/13	REVISION 8		
10	05/09/13	REVISION 9		
11	05/09/13	REVISION 10		
12	05/09/13	REVISION 11		
13	05/09/13	REVISION 12		
14	05/09/13	REVISION 13		
15	05/09/13	REVISION 14		
16	05/09/13	REVISION 15		
17	05/09/13	REVISION 16		
18	05/09/13	REVISION 17		
19	05/09/13	REVISION 18		
20	05/09/13	REVISION 19		
21	05/09/13	REVISION 20		
22	05/09/13	REVISION 21		
23	05/09/13	REVISION 22		
24	05/09/13	REVISION 23		
25	05/09/13	REVISION 24		
26	05/09/13	REVISION 25		
27	05/09/13	REVISION 26		
28	05/09/13	REVISION 27		
29	05/09/13	REVISION 28		
30	05/09/13	REVISION 29		
31	05/09/13	REVISION 30		
32	05/09/13	REVISION 31		
33	05/09/13	REVISION 32		
34	05/09/13	REVISION 33		
35	05/09/13	REVISION 34		
36	05/09/13	REVISION 35		
37	05/09/13	REVISION 36		
38	05/09/13	REVISION 37		
39	05/09/13	REVISION 38		
40	05/09/13	REVISION 39		
41	05/09/13	REVISION 40		
42	05/09/13	REVISION 41		
43	05/09/13	REVISION 42		
44	05/09/13	REVISION 43		
45	05/09/13	REVISION 44		
46	05/09/13	REVISION 45		
47	05/09/13	REVISION 46		
48	05/09/13	REVISION 47		
49	05/09/13	REVISION 48		
50	05/09/13	REVISION 49		
51	05/09/13	REVISION 50		
52	05/09/13	REVISION 51		
53	05/09/13	REVISION 52		
54	05/09/13	REVISION 53		
55	05/09/13	REVISION 54		
56	05/09/13	REVISION 55		
57	05/09/13	REVISION 56		
58	05/09/13	REVISION 57		
59	05/09/13	REVISION 58		
60	05/09/13	REVISION 59		
61	05/09/13	REVISION 60		
62	05/09/13	REVISION 61		
63	05/09/13	REVISION 62		
64	05/09/13	REVISION 63		
65	05/09/13	REVISION 64		
66	05/09/13	REVISION 65		
67	05/09/13	REVISION 66		
68	05/09/13	REVISION 67		
69	05/09/13	REVISION 68		
70	05/09/13	REVISION 69		
71	05/09/13	REVISION 70		
72	05/09/13	REVISION 71		
73	05/09/13	REVISION 72		
74	05/09/13	REVISION 73		
75	05/09/13	REVISION 74		
76	05/09/13	REVISION 75		
77	05/09/13	REVISION 76		
78	05/09/13	REVISION 77		
79	05/09/13	REVISION 78		
80	05/09/13	REVISION 79		
81	05/09/13	REVISION 80		
82	05/09/13	REVISION 81		
83	05/09/13	REVISION 82		
84	05/09/13	REVISION 83		
85	05/09/13	REVISION 84		
86	05/09/13	REVISION 85		
87	05/09/13	REVISION 86		
88	05/09/13	REVISION 87		
89	05/09/13	REVISION 88		
90	05/09/13	REVISION 89		
91	05/09/13	REVISION 90		
92	05/09/13	REVISION 91		
93	05/09/13	REVISION 92		
94	05/09/13	REVISION 93		
95	05/09/13	REVISION 94		
96	05/09/13	REVISION 95		
97	05/09/13	REVISION 96		
98	05/09/13	REVISION 97		
99	05/09/13	REVISION 98		
100	05/09/13	REVISION 99		
101	05/09/13	REVISION 100		