

# S1000-T2-H120 Rotary Vane Medical Vacuum System

System is NFPA compliant and has modular construction and interconnecting piping.

## PUMP MODULE

Oil sealed rotary vane vacuum pump with NEMA motor. Each pump module is equipped with an inlet filter, check valve, pump isolation valve, and temperature switch.

## SYSTEM CONTROLS

The UL listed electrical control panel features a high-definition color touch screen that can be set up externally without the use of toggle switches. The panel displays multiple conditions, including pump running status, elapsed hours, vacuum level, and audio/visual alarms.

Standard features include lag alarm, automatic pump alternation, adjustable minimum run timer, adjustable vacuum settings, adjustable screen brightness, alarm history registry, and data logging. The panel has standard dry contacts and Modbus interface with building management systems. Ethernet and BACnet are available as options. The panel's maintenance menu includes service items and maintenance warnings, and it is programmed for both English and Spanish languages.

## VACUUM RECEIVER

Constructed to ASME standards and rated for full vacuum. Equipped with valved bypass, high visibility vacuum gauge, source isolation valve, and a manual drain valve. Mounting pads and flex connectors supplied for field installation.

## KEY OPTIONS

Variable Speed Drive Electrical Panel  
Configurable for Lab or Industrial Applications  
Gas Purge System for Lab use

<b>Configuration</b>	Duplex Tank Mount
<b>System Capacity*</b>	71 SCFM @ 19" Hg. 60 Hz. 59 SCFM @ 19" Hg. 50 Hz.
<b>Horsepower (Each Pump)</b>	10 HP
<b>Horsepower (Total System)</b>	20 HP
<b>Available Voltage</b>	208/230/460V 3 PH 60 Hz. 380V 3 PH 50 Hz. Contact Factory for other voltages
<b>Full Load Amps 3 PH</b>	208 Volts: 62.8 230 Volts: 57.1 380 Volts: 34.8 460 Volts: 28.6
<b>Tank Size</b>	120 gallon horizontal
<b>Bacterial Filter Bank (option)</b>	BOM-MED FB-2




Click here for pump specifications  
and industry-leading parts support

\*System capacity is stated with one pump in reserve per NFPA. Capacity based on operation at sea level.  
For higher altitude, contact factory for adjusted capacity.

SYSTEM MODEL NO.	PART NO.	HP EACH	24" VACUUM 8" 1" 1/2" EACH	30" VACUUM 8" 2" 1/2" EACH	DESIGN CAPACITY (10" 1" 1/2" EACH)	RECOVERY SIZE (GALLONS)	PUMP INLET NPT	ESTIMATED SYSTEM WEIGHT (LB)
S1000-T2	S1000-460-T2-H120	10	71.1 / 174.6	29.4 / 174.4	21.5	120	2"	1900


SPACE ALLOWANCE FOR MAINTENANCE = 3 FT. ON ALL SIDES. MORE SPACE IS REQUIRED FOR THE OPENING OF LARGER PANEL DOOR.

TABLE 1			
SYSTEM LISTED ARE 480V. IF ANOTHER VOLTAGE IS REQUIRED, USE THE FOLLOWING PART NUMBERS.			
VOLTAGE	SYSTEM P/N	PUMP MODULE P/N	TRIP MODULE P/N
208-480-3	S1000-208-T2-H120	100-0204	21-4539
230-480-3	S1000-230-T2-H120	100-0204	21-4544
380-50-3	S1000-380-T2-H120	100-0204	21-4544


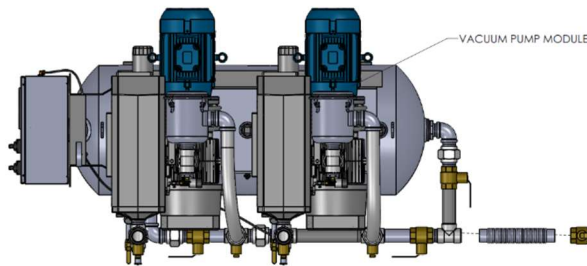


ELECTRICAL CONTROL PANEL

2" NPT EXHAUST CONNECTION

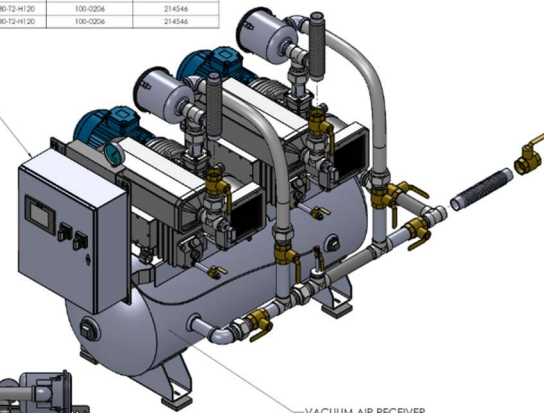

VACUUM AIR RECEIVER

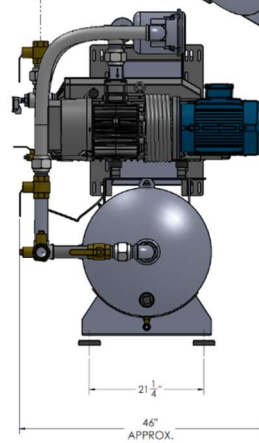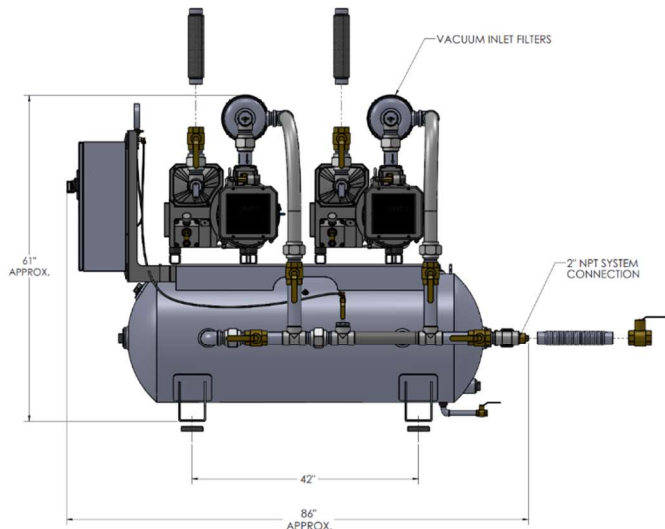

REV	DATE	DESCRIPTION	BY	CHK
1	02/14/18	INITIAL RELEASE	E. LOPEZ	02/14/18
2	02/14/18	REVISION	E. LOPEZ	02/14/18
3	02/14/18	REVISION	E. LOPEZ	02/14/18
4	02/14/18	REVISION	E. LOPEZ	02/14/18
5	02/14/18	REVISION	E. LOPEZ	02/14/18
6	02/14/18	REVISION	E. LOPEZ	02/14/18
7	02/14/18	REVISION	E. LOPEZ	02/14/18
8	02/14/18	REVISION	E. LOPEZ	02/14/18
9	02/14/18	REVISION	E. LOPEZ	02/14/18
10	02/14/18	REVISION	E. LOPEZ	02/14/18
11	02/14/18	REVISION	E. LOPEZ	02/14/18
12	02/14/18	REVISION	E. LOPEZ	02/14/18
13	02/14/18	REVISION	E. LOPEZ	02/14/18
14	02/14/18	REVISION	E. LOPEZ	02/14/18
15	02/14/18	REVISION	E. LOPEZ	02/14/18
16	02/14/18	REVISION	E. LOPEZ	02/14/18
17	02/14/18	REVISION	E. LOPEZ	02/14/18
18	02/14/18	REVISION	E. LOPEZ	02/14/18
19	02/14/18	REVISION	E. LOPEZ	02/14/18
20	02/14/18	REVISION	E. LOPEZ	02/14/18
21	02/14/18	REVISION	E. LOPEZ	02/14/18
22	02/14/18	REVISION	E. LOPEZ	02/14/18
23	02/14/18	REVISION	E. LOPEZ	02/14/18
24	02/14/18	REVISION	E. LOPEZ	02/14/18
25	02/14/18	REVISION	E. LOPEZ	02/14/18
26	02/14/18	REVISION	E. LOPEZ	02/14/18
27	02/14/18	REVISION	E. LOPEZ	02/14/18
28	02/14/18	REVISION	E. LOPEZ	02/14/18
29	02/14/18	REVISION	E. LOPEZ	02/14/18
30	02/14/18	REVISION	E. LOPEZ	02/14/18
31	02/14/18	REVISION	E. LOPEZ	02/14/18
32	02/14/18	REVISION	E. LOPEZ	02/14/18
33	02/14/18	REVISION	E. LOPEZ	02/14/18
34	02/14/18	REVISION	E. LOPEZ	02/14/18
35	02/14/18	REVISION	E. LOPEZ	02/14/18
36	02/14/18	REVISION	E. LOPEZ	02/14/18
37	02/14/18	REVISION	E. LOPEZ	02/14/18
38	02/14/18	REVISION	E. LOPEZ	02/14/18
39	02/14/18	REVISION	E. LOPEZ	02/14/18
40	02/14/18	REVISION	E. LOPEZ	02/14/18
41	02/14/18	REVISION	E. LOPEZ	02/14/18
42	02/14/18	REVISION	E. LOPEZ	02/14/18
43	02/14/18	REVISION	E. LOPEZ	02/14/18
44	02/14/18	REVISION	E. LOPEZ	02/14/18
45	02/14/18	REVISION	E. LOPEZ	02/14/18
46	02/14/18	REVISION	E. LOPEZ	02/14/18
47	02/14/18	REVISION	E. LOPEZ	02/14/18
48	02/14/18	REVISION	E. LOPEZ	02/14/18
49	02/14/18	REVISION	E. LOPEZ	02/14/18
50	02/14/18	REVISION	E. LOPEZ	02/14/18
51	02/14/18	REVISION	E. LOPEZ	02/14/18
52	02/14/18	REVISION	E. LOPEZ	02/14/18
53	02/14/18	REVISION	E. LOPEZ	02/14/18
54	02/14/18	REVISION	E. LOPEZ	02/14/18
55	02/14/18	REVISION	E. LOPEZ	02/14/18
56	02/14/18	REVISION	E. LOPEZ	02/14/18
57	02/14/18	REVISION	E. LOPEZ	02/14/18
58	02/14/18	REVISION	E. LOPEZ	02/14/18
59	02/14/18	REVISION	E. LOPEZ	02/14/18
60	02/14/18	REVISION	E. LOPEZ	02/14/18
61	02/14/18	REVISION	E. LOPEZ	02/14/18
62	02/14/18	REVISION	E. LOPEZ	02/14/18
63	02/14/18	REVISION	E. LOPEZ	02/14/18
64	02/14/18	REVISION	E. LOPEZ	02/14/18
65	02/14/18	REVISION	E. LOPEZ	02/14/18
66	02/14/18	REVISION	E. LOPEZ	02/14/18
67	02/14/18	REVISION	E. LOPEZ	02/14/18
68	02/14/18	REVISION	E. LOPEZ	02/14/18
69	02/14/18	REVISION	E. LOPEZ	02/14/18
70	02/14/18	REVISION	E. LOPEZ	02/14/18
71	02/14/18	REVISION	E. LOPEZ	02/14/18
72	02/14/18	REVISION	E. LOPEZ	02/14/18
73	02/14/18	REVISION	E. LOPEZ	02/14/18
74	02/14/18	REVISION	E. LOPEZ	02/14/18
75	02/14/18	REVISION	E. LOPEZ	02/14/18
76	02/14/18	REVISION	E. LOPEZ	02/14/18
77	02/14/18	REVISION	E. LOPEZ	02/14/18
78	02/14/18	REVISION	E. LOPEZ	02/14/18
79	02/14/18	REVISION	E. LOPEZ	02/14/18
80	02/14/18	REVISION	E. LOPEZ	02/14/18
81	02/14/18	REVISION	E. LOPEZ	02/14/18
82	02/14/18	REVISION	E. LOPEZ	02/14/18
83	02/14/18	REVISION	E. LOPEZ	02/14/18
84	02/14/18	REVISION	E. LOPEZ	02/14/18
85	02/14/18	REVISION	E. LOPEZ	02/14/18
86	02/14/18	REVISION	E. LOPEZ	02/14/18
87	02/14/18	REVISION	E. LOPEZ	02/14/18
88	02/14/18	REVISION	E. LOPEZ	02/14/18
89	02/14/18	REVISION	E. LOPEZ	02/14/18
90	02/14/18	REVISION	E. LOPEZ	02/14/18
91	02/14/18	REVISION	E. LOPEZ	02/14/18
92	02/14/18	REVISION	E. LOPEZ	02/14/18
93	02/14/18	REVISION	E. LOPEZ	02/14/18
94	02/14/18	REVISION	E. LOPEZ	02/14/18
95	02/14/18	REVISION	E. LOPEZ	02/14/18
96	02/14/18	REVISION	E. LOPEZ	02/14/18
97	02/14/18	REVISION	E. LOPEZ	02/14/18
98	02/14/18	REVISION	E. LOPEZ	02/14/18
99	02/14/18	REVISION	E. LOPEZ	02/14/18
100	02/14/18	REVISION	E. LOPEZ	02/14/18

